



EU Type Examination Certificate Number: 0120/SGS0213

Zhejiang Eastron Electronic Co., Ltd.

No.52, Dongjin Road
Nanhu
Jiaxing
Zhejiang
China

Instrument Identification:

SDM72D, SDM72DR, SDM72D-M-1, SDM72D-M-2, SDM72Bi

Polyphase, Active Import/Export (kWh), Electricity Meter

Instrument Traceable Number

0120/SGS0213

has been assessed and certified as meeting the requirements of

EU Directive 2014/32/EU on Measuring Instruments Annex II, Module B

It is certified that the manufacturer's technical design and specimen for the above instrument has been examined and, based on the evidence submitted, it is considered that the instrument conforms to the requirements of Annex V of EU Directive 2014/32/EU

This certificate must be used in conjunction with a certificate covering the product verification as required in Annex II, Module D or Annex II, Module F

This certificate is valid until 20th April 2026
Issue 2

Certification is based on report number(s):

Certification is based on report number(s): SHES151000648101 dated 19th April 2016
EMA288418/1 dated 1st April 2021, EMA288737/3 dated 1st April 2021, EMA288418.1p2w dated 4th July 2022

Authorised Signature

Mikko Välimäki

SGS Fimko OY, Notified Body 0598
Takomatie 8, FI-00380 Helsinki, Finland
t +358 9 6963 61 www.sgs.fi




	EU-Type Examination Certificate Number:	
	0120/SGS0213	
	Issue Number: 3	Dated: 04 October 2023

1. Technical Data

Manufacturer	Zhejiang Eastron Electronic Co Ltd
Meter Type	SDM72D, SDM72DR, SDM72D-M-1, SDM72D-M-2, SDM72Bi
Voltage Rating (U_n)	230V & 3 x 230/400V
Current Rating (I_{min} – I_{ref} (I_{max}))	0,5-10(100)A & 0.5-10(80)A
Frequency (F_n)	50Hz
Active Accuracy Class (kWh)	B (kWh)
Type of circuit	3p4w, 1p2w
Temperature Range	-25°C to +55°C or -40°C to +70°C
Software/ Firmware Version No's	SDM72D: V1.1 SDM72DR: V1.1 SDM72Bi: V1.1 SDM72D-M-1: V1.3 SDM72D-M-2: V1.3
CRC Checksum No.s	SDM72D: EA8DA16C SDM72DR: 3BB6108A SDM72Bi: F02A9803 SDM72D-M-1: 9E71902C SDM72D-M-2: 9E71902C
Identification Location	Laser printed on meter case
Bill of Materials No's	SDM72D : DH-JS-150050 V1.4 SDM72DR : DH-JS-160007 V1.5 SDM72BI : DH-JS-160007 V1.5 SDM72D-M-1 : DH-JS-200010 V1.2 SDM72D-M-2 : DH-JS-200010 V1.2
IP Rating	IP51
Insulation Protective Class	Class II
LED Pulse Constant	1000 imp/kWh or 100imp/kWh
Impulse Voltage Rating	6kV
AC Voltage Rating	4kV
Main Cover Sealing Type	Wire & Crimp on terminal cover Meter case sealed with screws
Integrity of meter	Inaccessible without breaking seals
Intended Location of the Meter	Indoor
Type of Register	LCD
Terminal Arrangement(s)	DIN
Location of Manufacturers Address	Associated documents

	EU-Type Examination Certificate Number:	
	0120/SGS0213	
	Issue Number: 3	Dated: 04 October 2023

2. Photograph of Meter and Sealing Plan

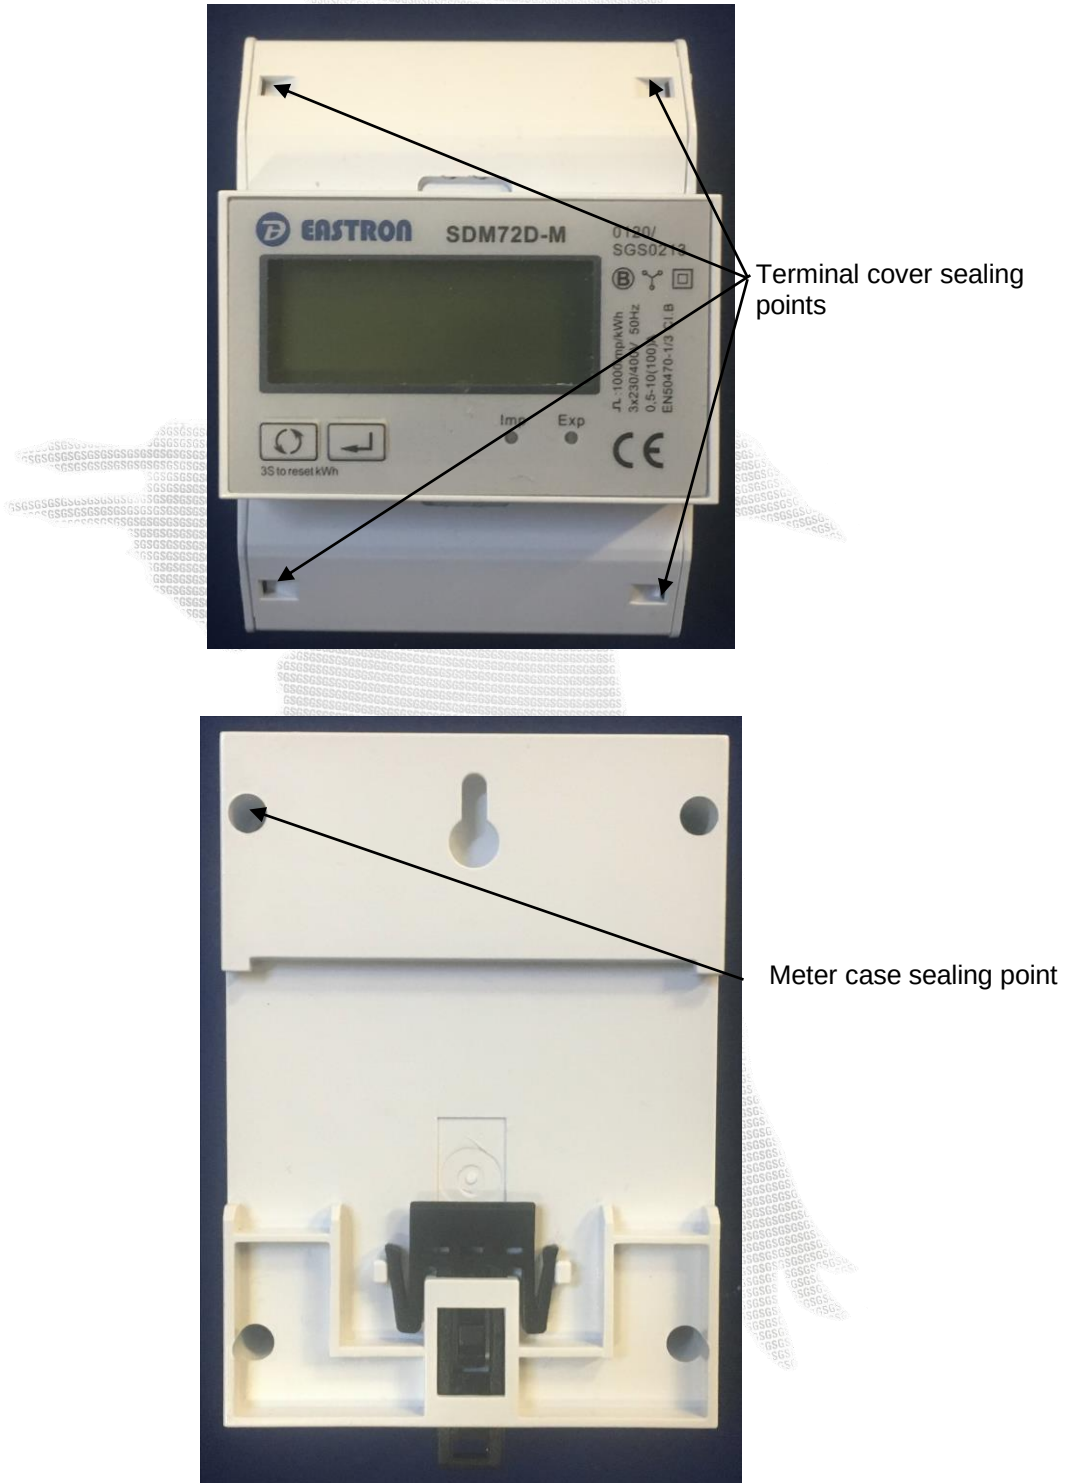

	EU-Type Examination Certificate Number:	
	0120/SGS0213	
	Issue Number: 3	Dated: 04 October 2023

3. Examples of Nameplates



Eastron
SDM72Bi 0120/SGS0213
Three Phase Energy Meter
3x230/400V~ 0.5-10(100)A 50Hz 2023
1000imp/kWh EN50470-1/3 IP51 SW:V1.1 CAT III
UK M23 CE M23 B □ Y △ 3K6
Manufactured by Zhejiang Eastron Electronic Co., Ltd.
No. 52, Dongjin Road, Nanhu, Jiaxing, Zhejiang, China

Eastron
SDM72Bi 0120/SGS0213
Three Phase Energy Meter
3x230/400V~ 0.5-10(100)A 50Hz 2023
1000imp/kWh EN50470-1/3 IP51 SW:V1.1 CAT III
UK M23 CE M23 B □ Y △ 3K7
Manufactured by Zhejiang Eastron Electronic Co., Ltd.
No. 52, Dongjin Road, Nanhu, Jiaxing, Zhejiang, China



Eastron
SDM72D 0120/SGS0213
Three Phase Energy Meter
3x230/400V~ 0.5-10(100)A 50Hz 2023
1000imp/kWh EN50470-1/3 IP51 SW:V1.1 CAT III
UK M23 CE M23 B □ Y △ 3K6
Manufactured by Zhejiang Eastron Electronic Co., Ltd.
No. 52, Dongjin Road, Nanhu, Jiaxing, Zhejiang, China

Eastron
SDM72D 0120/SGS0213
Three Phase Energy Meter
3x230/400V~ 0.5-10(100)A 50Hz 2023
1000imp/kWh EN50470-1/3 IP51 SW:V1.1 CAT III
UK M23 CE M23 B □ Y △ 3K7
Manufactured by Zhejiang Eastron Electronic Co., Ltd.
No. 52, Dongjin Road, Nanhu, Jiaxing, Zhejiang, China



Eastron
SDM72DR 0120/SGS0213
Three Phase Energy Meter
3x230/400V~ 0.5-10(100)A 50Hz 2023
1000imp/kWh EN50470-1/3 IP51 SW:V1.1 CAT III
UK M23 CE M23 B □ Y △ 3K6
Manufactured by Zhejiang Eastron Electronic Co., Ltd.
No. 52, Dongjin Road, Nanhu, Jiaxing, Zhejiang, China

Eastron
SDM72DR 0120/SGS0213
Three Phase Energy Meter
3x230/400V~ 0.5-10(100)A 50Hz 2023
1000imp/kWh EN50470-1/3 IP51 SW:V1.1 CAT III
UK M23 CE M23 B □ Y △ 3K7
Manufactured by Zhejiang Eastron Electronic Co., Ltd.
No. 52, Dongjin Road, Nanhu, Jiaxing, Zhejiang, China

SGS

EU-Type Examination Certificate Number:

0120/SGS0213

Issue Number: 3

Dated: 04 October 2023



Eastron

SDM72D-M-1 0120/SGS0213
Three Phase Energy Meter

3x230/400V~ 0.5-10(100)A 50Hz 2023
1000imp/kWh EN50470-1/3 IP51 SW:V1.3 CAT III

UK M23 CE M23 B □ ↓ Y △ 3K6

Manufactured by Zhejiang Eastron Electronic Co., Ltd.
No. 52, Dongjin Road, Nanhu, Jiaxing, Zhejiang, China

Eastron

SDM72D-M-1 0120/SGS0213
Three Phase Energy Meter

3x230/400V~ 0.5-10(100)A 50Hz 2023
1000imp/kWh EN50470-1/3 IP51 SW:V1.3 CAT III

UK M23 CE M23 B □ ↓ Y △ 3K7

Manufactured by Zhejiang Eastron Electronic Co., Ltd.
No. 52, Dongjin Road, Nanhu, Jiaxing, Zhejiang, China

Eastron

SDM72D-M-2 0120/SGS0213
Three Phase Energy Meter

3x230/400V~ 0.5-10(100)A 50Hz 2023
1000imp/kWh EN50470-1/3 IP51 SW:V1.3 CAT III

UK M23 CE M23 B □ ↓ Y △ 3K6

Manufactured by Zhejiang Eastron Electronic Co., Ltd.
No. 52, Dongjin Road, Nanhu, Jiaxing, Zhejiang, China

Eastron

SDM72D-M-2 0120/SGS0213
Three Phase Energy Meter

3x230/400V~ 0.5-10(100)A 50Hz 2023
1000imp/kWh EN50470-1/3 IP51 SW:V1.3 CAT III

UK M23 CE M23 B □ ↓ Y △ 3K7

Manufactured by Zhejiang Eastron Electronic Co., Ltd.
No. 52, Dongjin Road, Nanhu, Jiaxing, Zhejiang, China

	EU-Type Examination Certificate Number:	
	0120/SGS0213	
	Issue Number: 3	Dated: 04 October 2023

4. Calculation of the composite error/ MPE

During the type approval examination the influence factors for temperature, frequency and voltage are determined per load point. The table below represents the sum of the square values per load, determined via the following formula:-

$$\delta e(T, U, f) = \sqrt{(\delta e^2(T, I, \cos\phi) + \delta e^2(U, I, \cos\phi) + \delta e^2(f, I, \cos\phi))}$$

where

$\delta e(T, I, \cos\phi)$ = Additional error due to variation of the temperature at the same load
 $\delta e(U, I, \cos\phi)$ = Additional error due to variation of the voltage at the same load
 $\delta e(f, I, \cos\phi)$ = Additional error due to variation of the frequency at the same load

1P2W Configuration

		Influence Factors for temperature, frequency and voltage							
Current	PF Cos	-40°C	-25°C	-10°C	5°C	30°C	40°C	55°C	70°C
I _{min}	1.0	0.10	0.11	0.11	0.07	0.08	0.12	0.17	0.21
I _{tr}	1.0	0.07	0.10	0.10	0.06	0.05	0.09	0.15	0.19
10I _{tr}	1.0	0.05	0.08	0.08	0.05	0.06	0.09	0.15	0.19
I _{max}	1.0	0.18	0.14	0.08	0.03	0.09	0.12	0.15	0.16
I _{tr}	0.5ind	0.12	0.13	0.12	0.07	0.07	0.11	0.15	0.19
10I _{tr}	0.5ind	0.05	0.08	0.08	0.05	0.07	0.10	0.15	0.18
I _{max}	0.5ind	0.11	0.07	0.02	0.07	0.17	0.20	0.22	0.22
I _{tr}	0.8cap	0.12	0.14	0.14	0.09	0.03	0.07	0.12	0.16
10I _{tr}	0.8cap	0.07	0.10	0.10	0.06	0.05	0.08	0.14	0.17
I _{max}	0.8cap	0.19	0.15	0.09	0.04	0.07	0.11	0.14	0.14



EU-Type Examination Certificate Number:

0120/SGS0213

Issue Number: 3

Dated: 04 October 2023

3P4W Configuration

		Influence Factors for Temperature. Frequency & Voltage							
Current	PF Cos	-40°C	-25°C	-10°C	5°C	30°C	40°C	55°C	70°C
I _{min}	1.0	0.08	0.32	0.24	0.15	0.12	0.15	0.26	0.70
I _{tr}	1.0	0.13	0.34	0.24	0.15	0.10	0.15	0.30	0.61
10I _{tr}	1.0	0.26	0.37	0.28	0.17	0.10	0.15	0.28	0.51
I _{max}	1.0	0.12	0.30	0.24	0.19	0.15	0.17	0.24	0.44
I _{tr}	0.5ind	0.26	0.51	0.45	0.37	0.30	0.30	0.36	0.59
10I _{tr}	0.5ind	0.34	0.40	0.32	0.25	0.18	0.22	0.32	0.43
I _{max}	0.5ind	0.45	0.66	0.62	0.58	0.52	0.51	0.50	0.40
I _{tr}	0.8cap	0.18	0.44	0.34	0.26	0.16	0.17	0.24	0.62
10I _{tr}	0.8cap	0.19	0.37	0.25	0.15	0.09	0.15	0.27	0.56
I _{max}	0.8cap	0.27	0.48	0.42	0.38	0.33	0.31	0.32	0.44
L1									0.00
I _{tr}	1.0	0.19	0.37	0.33	0.29	0.26	0.28	0.38	0.93
10I _{tr}	1.0	0.08	0.30	0.21	0.15	0.10	0.17	0.29	1.09
I _{max}	1.0	0.29	0.23	0.18	0.17	0.11	0.14	0.23	1.09
I _{tr}	0.5ind	0.15	0.44	0.38	0.35	0.34	0.38	0.44	1.16
10I _{tr}	0.5ind	0.19	0.31	0.24	0.22	0.19	0.26	0.38	1.25
I _{max}	0.5ind	0.31	0.29	0.26	0.25	0.22	0.24	0.34	1.08
L2									
I _{tr}	1.0	0.21	0.61	0.61	0.61	0.61	0.61	0.61	0.68
10I _{tr}	1.0	0.11	0.19	0.19	0.19	0.19	0.19	0.20	0.49
I _{max}	1.0	0.30	0.16	0.14	0.12	0.12	0.12	0.12	0.50
I _{tr}	0.5ind	0.53	0.76	0.77	0.77	0.76	0.77	0.77	1.00
10I _{tr}	0.5ind	0.48	0.31	0.30	0.30	0.30	0.31	0.32	0.97
I _{max}	0.5ind	0.66	0.30	0.28	0.27	0.27	0.27	0.27	0.85
L3									
I _{tr}	1.0	0.46	0.80	0.52	0.38	0.27	0.37	0.54	0.17
10I _{tr}	1.0	0.70	0.86	0.64	0.50	0.42	0.48	0.63	0.14
I _{max}	1.0	0.71	1.09	0.97	0.90	0.87	0.89	0.95	0.68
I _{tr}	0.5ind	1.40	1.04	0.92	0.82	0.79	0.82	0.92	0.93
10I _{tr}	0.5ind	1.58	1.03	0.88	0.78	0.74	0.78	0.88	1.03
I _{max}	0.5ind	1.24	1.02	0.92	0.92	0.83	0.87	0.94	1.08

	EU-Type Examination Certificate Number:	
	0120/SGS0213	
	Issue Number: 3	Dated: 04 October 2023

5. Annex of Variants

Product Variant Identification Details:

Type Designation	Description of meter
SDM72D	3x230/400V, 0.5-10(100)A or 0.5-10(80)A 1000imp/kWh or 100imp/kWh Shows only total active energy, without resettable kWh
SDM72DR	3x230/400V, 0.5-10(100)A or 0.5-10(80)A 1000imp/kWh or 100imp/kWh Shows total active energy, resettable kWh, total active power
SDM72D-M-1	230V or 3x230/400V, 0.5-10(100)A or 0.5-10(80)A 1000imp/kWh or 100imp/kWh Shows total active energy, total active power, import and export energy, resettable import and export energy. RS485 communication.
SDM72D-M-2	230V or 3x230/400V, 0.5-10(100)A or 0.5-10(80)A 1000imp/kWh or 100imp/kWh Shows total active energy, total active power, import and export energy, resettable import and export energy, voltage, current, power factor, frequency and demand values. RS485 communication.
SDM72Bi	3x230/400V, 0.5-10(100)A or 0.5-10(80)A 1000imp/kWh or 100imp/kWh Shows total active energy, total active power, import and export energy, resettable import and export energy

Modifications to the meter(s) described according to approval No.**0120/SGS0213** must be notified to the issuing body to confirm the meter(s) continuing compliance to the relevant pattern approval standard(s).

	EU-Type Examination Certificate Number:	
	0120/SGS0213	
	Issue Number: 3	Dated: 04 October 2023

6. Document Revision History

Issue	Date	Comments
1	21/04/2016	Initial Issue
2	18/07/2016	Revised BOM numbers
3	26/03/2018	Model SDM72D-M added to approval
4	07/05/2019	Additional variants 0.5-10(80)A added to approval
5	07/08/2019	Meter constant 100imp/kWh variant added to approval
6	08/04/2021	Replace meter variant SDM72D-M with SDM72D-M-1 & SDM72D-M-2 Update. BOM number and Software number for these two variants. Temperature range updated to -40°C to +70°C. Change of notified body reference.
1	12/07/2022	Issue 1 for SGS Fimko NB 0598 The original approval certificate issued 21/04/2016 The modifications listed above were made prior to the transfer to SGS Fimko 1P2W wiring configuration option for SDM72-M-1 and SDM72-M-2
2	12/07/2022	Minor firmware change for serial output. Software version V1.3 remains the same. New CRC number 0388
3	04/10/2023	Company address change to new address Nameplate and side nameplate change Add CRC checksum numbers BoM numbers update

This document is issued by the Company subject to its General Conditions for Certification Services, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>.

Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 28 days only.

END OF CERTIFICATE